

FIG. 1

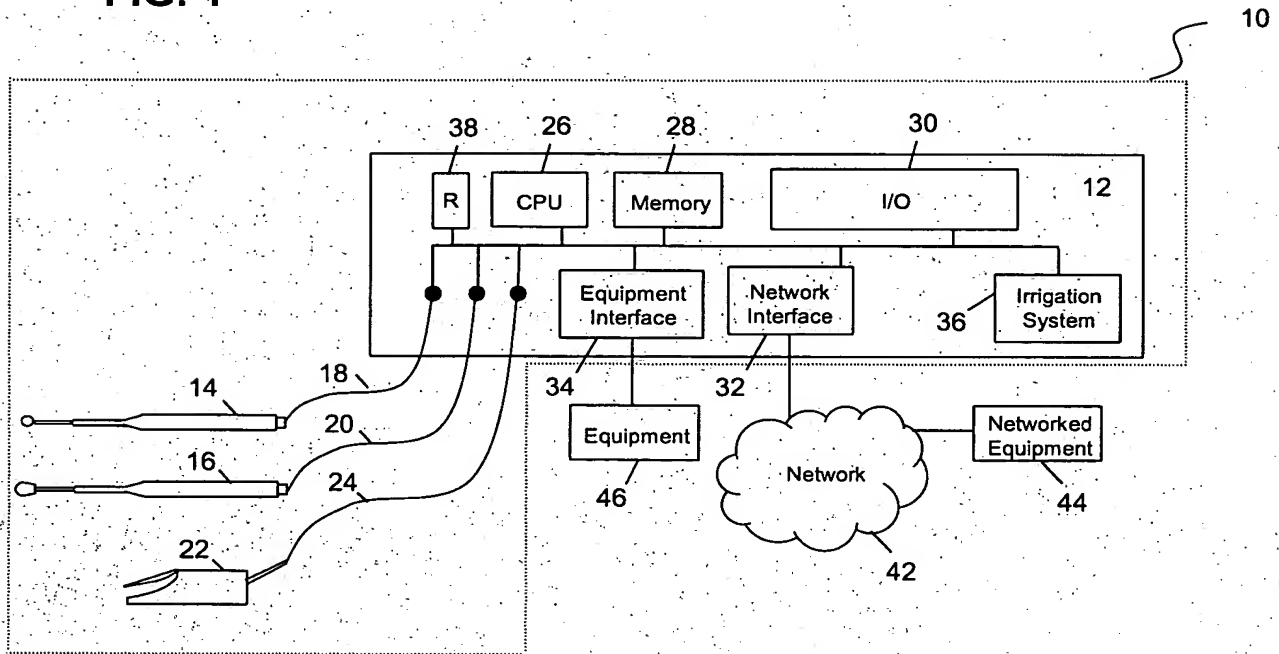


FIG. 2

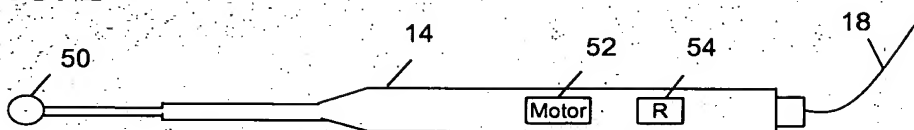


FIG. 3

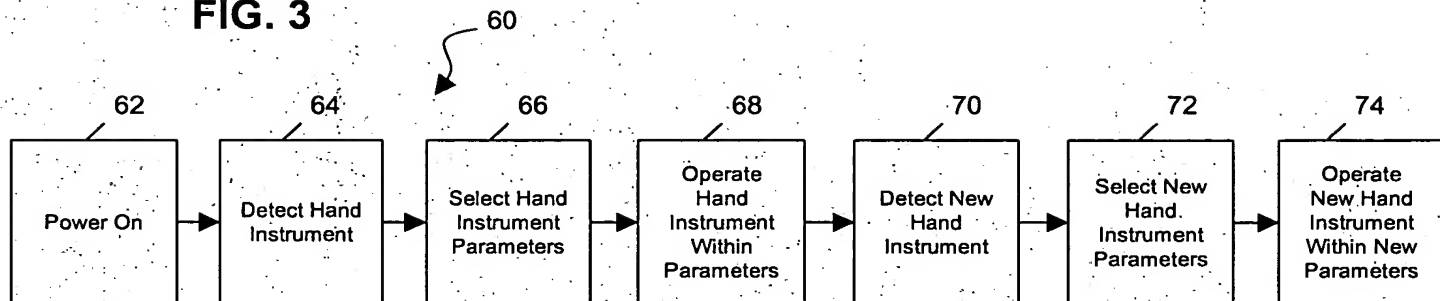


FIG. 4

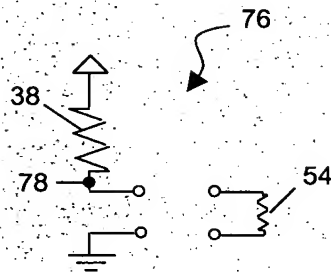


FIG. 5

Hand Instrument	Voltage Value	Signature Resistor	Parameter A	Parameter B	...
HI ₁₄	V ₇₈	R ₅₄	PA _n	PB _n	...
HI _n	V _n	R _n	PA _n	PB _n	...

Table 80 lists parameters for different hand instruments. The columns are: Hand Instrument, Voltage Value, Signature Resistor, Parameter A, Parameter B, and ... The rows show specific parameters for HI₁₄ and HI_n.

FIG. 6

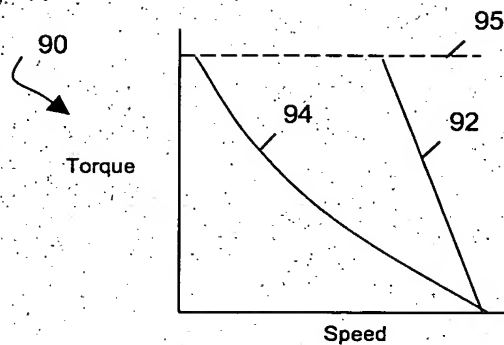


FIG. 7

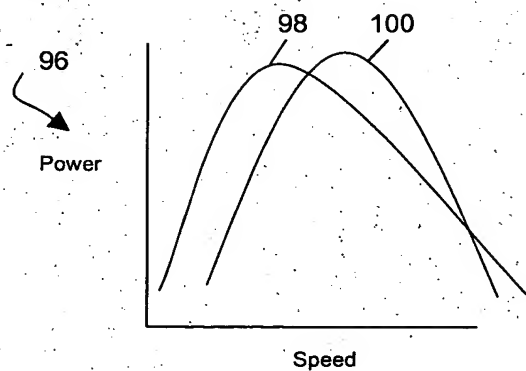


FIG. 8

